

Using a Density Sensor for Fuel Quality Monitoring

1. Introduction

Oil prices spikes and growing alternative fuel use, have given rise to opportunities for new sensing technology. New fuels like ethanol, biodiesel, butanol and Fischer-Tropsch fuel are all finding an increase in both gallons produced and the number of applications previously left to petrochemicals (1-14). Cost pressures and the array of biofuels are generating new markets for sensors to assist in fuel blending, indentifying fuel type, conversion to mass from volumetric inflow, and insuring fuel quality. Different petrochemicals and the new alternative fuels have different density values, as shown in Table 1. ISSYS has developed a unique fuel concentration / density sensor that can satisfy the requirements for the petrochemical and emerging alternative energy fuel market at an affordable price. This new sensor is based on a MEMS

(MicroElectroMechanical Systems) sensing chip that has already been developed for the laboratory, industrial and fuel cell concentration sensing applications (15-18). Other MEMS devices have been adapted to severe, high-volume, relatively low cost applications in the automotive (19), consumer and medical markets so we are confident that this technology will provide both a technical and commercial solution for fuel quality, custody transfer and blending sensing applications.

Fuel	Density Range (gm/cc)
Gasoline	0.725-0.775
E85	0.775-0.782
Ethanol	0.7856
Butanol	0.8095
Fisher Tropsch "diesel"	0.784-0.801
Diesel	0.822-0.860
Biodiesel	0.860-0.900

Table 1. Density ranges of various liquid fuels.

2. Alternative Energy Fuel Markets

2.1 Ethanol Market

Ethanol is the most established biofuel market, with an early start in Brazil (10) and a more recent expansion into the US (4-9). Figure 1 shows a map of ethanol production plants in the US. Figure 2 shows how fast the US ethanol production capacity has increased between 1999 and 2007. Truly high ethanol capacity will require the development of a non-food

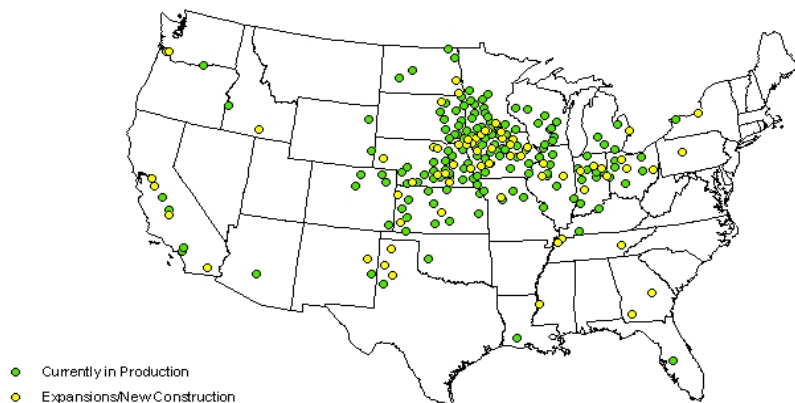


Figure 1. Ethanol production plants and those under construction, May 2008 (7)

feedstock, which is underway. While ethanol can reduce imported oil, it does have

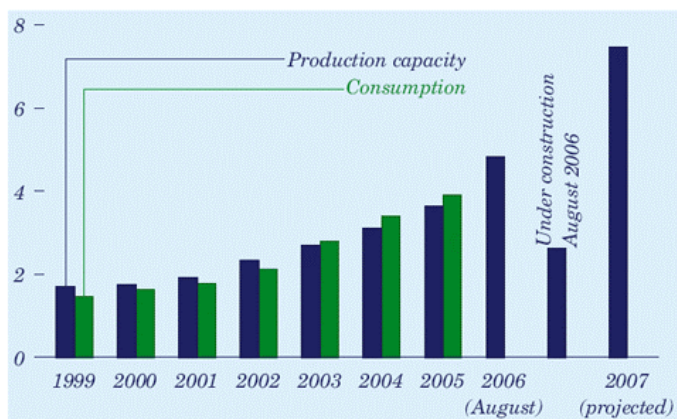


Figure 2. US ethanol production and capacity 1999-2007 in billions of gallons (9).



Figure 3. Blending fuel tanks: ethanol and gasoline (8).

disadvantages in lower gas mileage and contributing to the corrosion of the fuel system. To improve gas mileage ethanol is generally blended with gasoline. Ten and eighty five percent ethanol are the most common blends. As is shown in Figure 3, blending of ethanol and gasoline is already being developed to cover an even wider range of concentrations. Two tank systems one with ethanol and one with gasoline can be used to generate a wide variety of fuel blends.

Corrosion issues are due ethanol's ability to absorb and dissolve water. It is the water that leads to tank, pipeline and fuel line corrosion. This requires more expensive metals/alloys to be used in vehicles and prevents pipelines from being used to transport ethanol. Butanol (11) is an alternative to ethanol that can be distilled from the same feedstock. Butanol does not absorb water as readily as ethanol so could be transported like petrochemicals via a pipeline system. As Table 1 indicates, butanol can be distinguished from ethanol and gasoline via a density measurement.

2.2 Biodiesel Market

The biodiesel is behind the ethanol market volume in the US, but actually is the leading biofuel market in Europe due to their higher reliance on diesel fuel. Like ethanol, biodiesel is being used in blends with petrochemicals for its initial introduction into the market place. Table 2 shows the US market for blended ethanol and biodiesel in 2005. The 5 to 20% biofuel

Fuel	Production	Motor fuel consumption	Blend	Current blend consumption
Ethanol	3.90	136.9	E10	13.70
Biodiesel	0.08	43.2	B2	0.86
			B5	2.16
			B20	8.64

Table 2. US market for biofuel blends as of 2005 in billion of gallons (9).

Fuel	Number of stations	Percent of total
All fuels	169,000	100.0
Biofuels	1,767	1.0
E85	799	0.5
Biodiesel	968	0.5

Table 3. Vehicle fueling stations in the US as of 2006 (9).

concentration are the most common blends on the market. As Table 1 shows, biodiesel has a higher density than petrochemical diesel. Biodiesel has poorer cold temperature performance, but improved fuel lubricity and can improve exhaust emissions (20). The number of fuel filling stations and those that already accommodate biofuels are given in Table 3. The total number of filling stations in the US is 169,000. Almost 1000 stations are capable of pumping biodiesel. Table 4 gives the total number of gallons of motor fuel consumed annually in the US and what percentage in a biofuel. Ethanol is up over 2%, but biodiesel is less than a quarter of a percent of the total volume consumed. The capacity for growth clearly exists for both biofuels. Figure 4 show the world capacity for biodiesel production. As experience accumulates in this industry, larger facilities are being manufactured by a wider array of industrial. Rapid growth is projected here and abroad. Larger fuel processing capacity will drive wide use, leading to more filling stations, tanker trucks and vehicles employing biofuels.

	<i>Gasoline</i>	<i>Ethanol</i>	<i>Percent of gasoline pool</i>
2000	128,662	1,630	1.27
2001	129,312	1,770	1.37
2002	132,782	2,130	1.60
2003	134,089	2,800	2.09
2004	137,022	3,400	2.48
2005	136,949	3,904	2.85
	<i>Diesel</i>	<i>Biodiesel</i>	<i>Percent of diesel fuel pool</i>
2000	37,238	—	—
2001	38,155	9	0.02
2002	38,881	11	0.03
2003	40,856	18	0.04
2004	42,773	28	0.07
2005	43,180	91	0.21

Table 4. US motor fuel consumption in millions of gallons per year, for 2000-2005 (9).

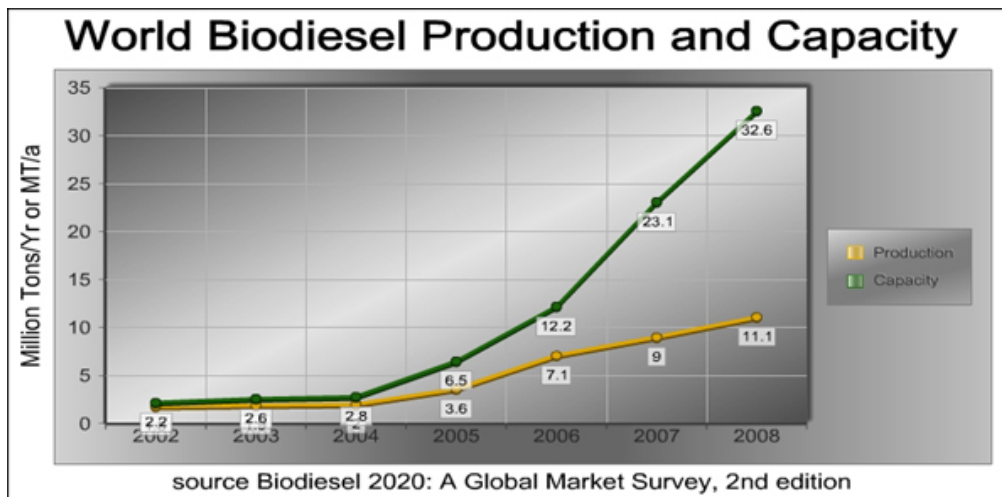


Figure 4. World biodiesel production and capacity through 2008 (12).

2.3 Fisher-Tropsch Fuel

A potential long term solution to the US dependence on Middle Eastern oil imports is the development of Fisher-Tropsch (FT) fuels. These liquid fuels are produced from hydrocarbon feedstock like coal, natural gas or oil shale. Due to higher processing costs, the development and use of Fisher-Tropsch fuel has to date been limited to countries with import barriers for petrochemicals such as South Africa during apartheid and Germany during World War II, or an excess of natural gas resources such as modern Malaysia (1). The US military has taken the lead in this area with a long term goal on replacing 75% of the oil imports by 2025 (1,2). These reserves offer the equivalent oil reserve of 2.3Trillion barrels, more than three times the Middle East oil reserves. The main measureable difference between Fisher-Tropsch fuel and petrochemical fuel is density. As Table 1 showed, FT fuel can be distinguished from petrochemical diesel fuel and biodiesel by density. The US military is introducing this fuel into military aviation and trucking, commercial aviation and trucking will follow with automotive applications being the last adopter of this alternative fuel.

2.4 Petrochemical Market

The majority of the existing fuel applications are with petrochemicals. Density goes down as you move up the distillation column as illustrated in Figure 5. Petrochemicals are already blended with each other to produce different grades of gasoline and diesel fuels. They

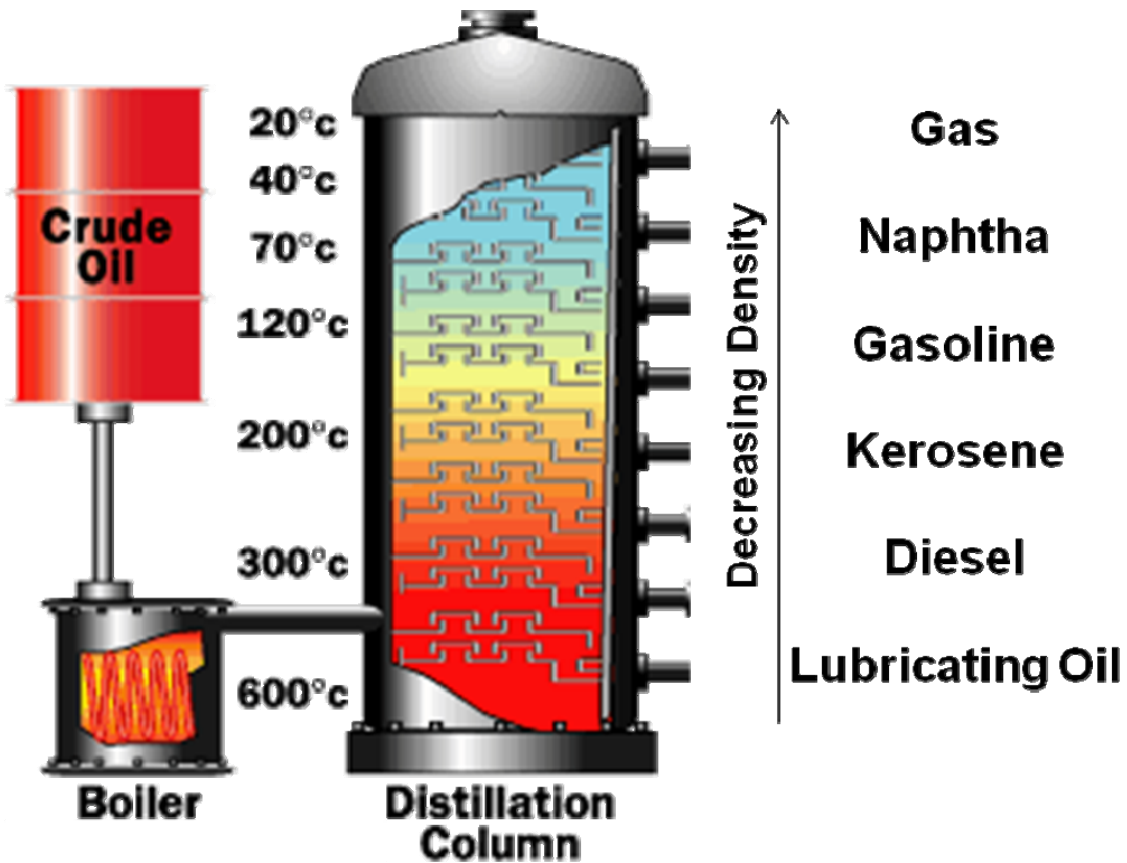


Figure 5. The petrochemical and density change along a distillation column.

are also blended with biofuels like ethanol and biodiesel. Density measurement of aviation is critical for custody transfer. Oil companies sell fuel volumetrically, while aircraft use mass-based measurement. Fuel temperature and blend quality causes the density to change which affects the fuel mass delivered to aircraft and in many cases can put the airlines at a cost disadvantage, particularly in hot conditions.

3. ISSYS' Density Sensors

ISSYS has developed a unique fluid density sensor based on its patented micromachined density and flow sensor technology. ISSYS began selling density and concentration meters using this MEMS-based technology in 2003 (15,16). This sensing approach uses a small, hollow silicon microtube. This small tube vibrates at a given frequency, as the density or concentration of the liquid in the tube changes the vibration frequency will change. The ISSYS model FC6 in-line density meter and Fuel Cell sensor, shown in Figure 6, was first applied to measuring methanol concentration in a DMFC system. This new sensor provides a needed device for the Direct Methanol Fuel Cell (DMFC) market (21,22). Without an accurate methanol concentration sensor, active DMFCs cannot perform efficiently.

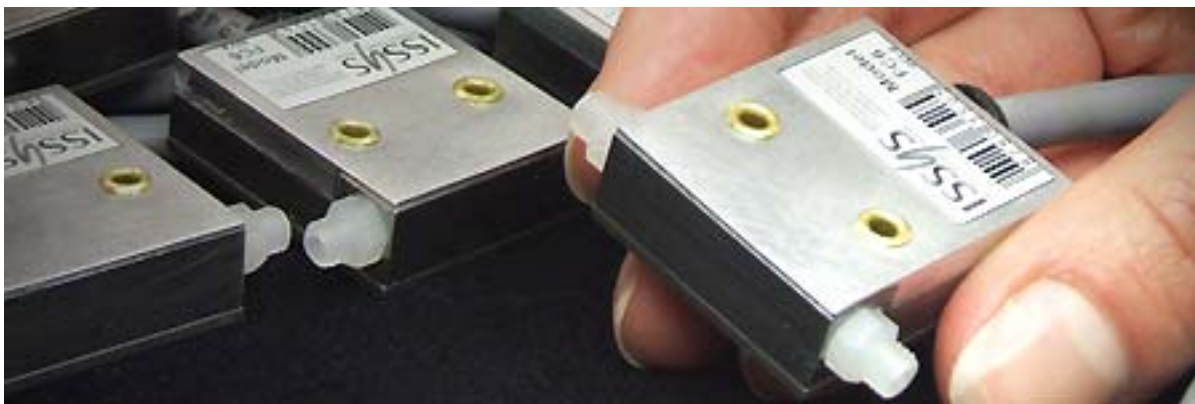


Figure 6. The ISSYS FC-6 density and chemical concentration sensor.

The sensing concept is universal for virtually any fluid or liquid solution. The density of the fluid (liquid or gas) can be measured using the vibrational frequency of the microtube. For binary solutions this has been used with methanol and ethanol, fuel cells to measure concentration. Petrochemicals and biofuels can use the density or API output to indicate the type of fuel, its purity and to blend fuels together. Fig 7 shows an intrinsically safe density sensor designed by ISSYS. The ISDS-08 can be used with all types of liquid fuels and fuel blends.

There are no other products on the market that can accurately identify fuel type, sense fuel concentration for blending over a wide temperature and concentration range and in the presence of chemical impurities for the size and cost the ISSYS device can achieve. ISSYS' proprietary, patented MEMS-based technologies are the key to making this type of device possible.



Figure 7. The intrinsically safe ISDS-08 density sensor.

3.1 ISSYS' MEMS Sensor Technology

The ISSYS resonant microtubes employ a MEMS fabrication process, which uses a combination of plasma and wet etching, photolithography, along with wafer bonding to form their microfluidic chips (15). Figure 8 shows an uncapped microtube resonator chip. The silicon tube, shown in Figure 8, is anodically bonded to glass. This glass wafer has the metal electrodes and runners used to carry electrical signals. The metal layer is also used as an on-chip, resistive temperature sensor. Two holes in the bottom glass chip admit fluid into and out of the silicon microtube.

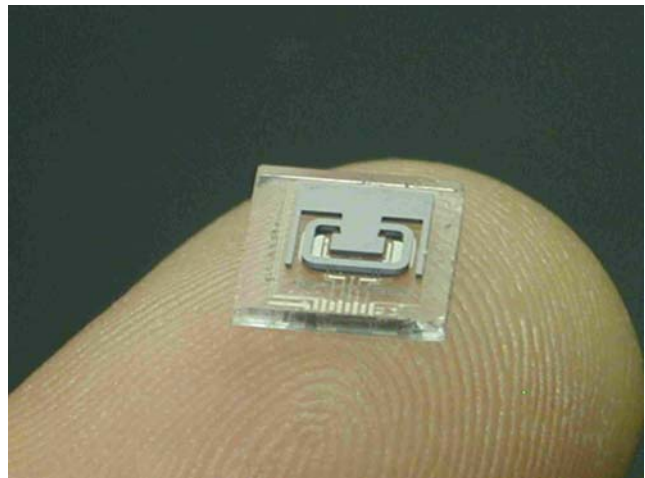


Figure 8. A decapped, MEMS chip, on a finger tip, showing the microtube and metal pattern.

The MEMS chip requires electronics to amplify the signal and drive the microtube into resonance, in addition the signal is processed to obtain a methanol concentration value. The tube is driven into resonance electrostatically and its motion sensed capacitively using metal electrodes under the tube and accompanying electronic circuits connected to the MEMS chip via wire bonding.

3.2 ISSYS Sensor Performance Results

The density of any fluid varies with temperature. For example, the characterization of methanol to water concentration over temperature is key to arriving at an accurate methanol concentration value. Figure 9 shows how the density of diesel fuel varies over temperature. Similar relationships exist for different fuels.

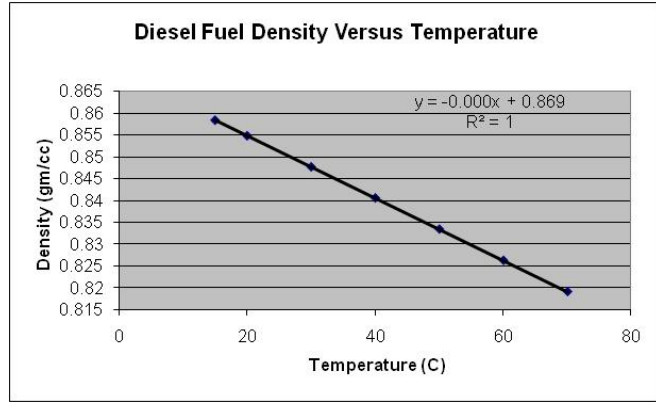


Figure 9. The variation in density of diesel fuel over temperature.

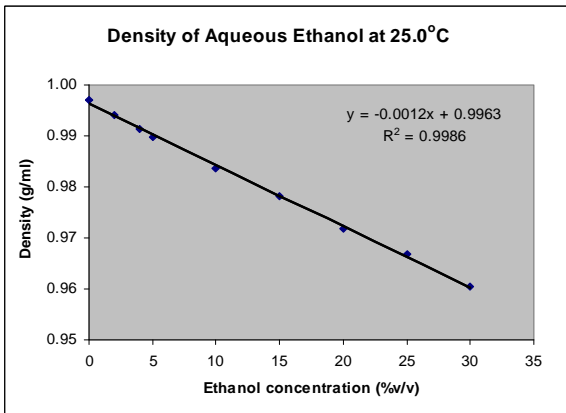


Figure 10. A density versus concentration plot for ethanol and water, data taken with the ISSYS MEMS sensor (16).

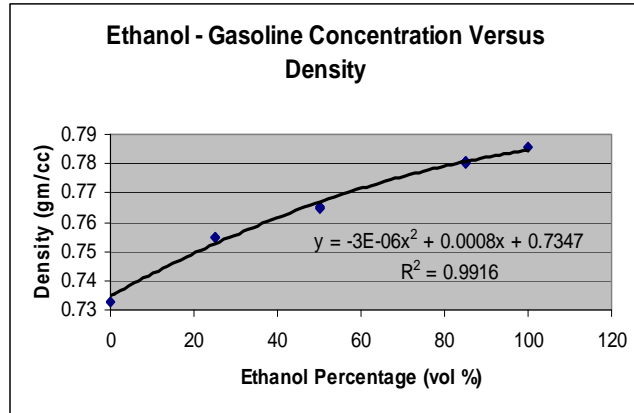


Figure 11. The density plot for ethanol-gasoline at 25°C.

A variety of fuels can employ density and flow sensors. Table 1 shows how the density of various biofuels and petrochemicals compare. Density can be used as an effective fuel identifier and for blending purposes. Figure 9 shows how diesel fuel density varies with temperature. Figure 10 and 11 show how the concentration of water or gasoline in ethanol can be measured using density. Water has a higher density than ethanol while gasoline has a lower density than ethanol. In ethanol refining and transportation water contamination is a big problem that leads to fuel system corrosion and poor fuel efficiency. ISSYS has sold a number of density meters to the ethanol refining industry as a quality sensor for water contamination.

Table 5 shows that density can also be used to detect water and air bubbles in a liquid and can be used to monitor the quality of antifreeze and hydraulic fluid. Water contamination can be a problem with pipe transport and tank storage. Trapped water at the bottom of a fuel tank can be detected via density.

Table 5 Densities of other fluids.	
Fluid (15.55°C)	Density (gm/cc)
Coolant/Antifreeze	1.12622
Water	0.99904
Hydraulic Fluid	0.87058
Kerosene	0.85450
Diesel Fuel	0.82258
Methanol	0.79592
Air	0.00122

4. Comparisons to Steel Coriolis Mass Flow and Density Meters

Stainless steel resonating Coriolis mass flow meters and density meters are made by a variety of manufactures, shown in Figure 12. Price, size and weight are the main force

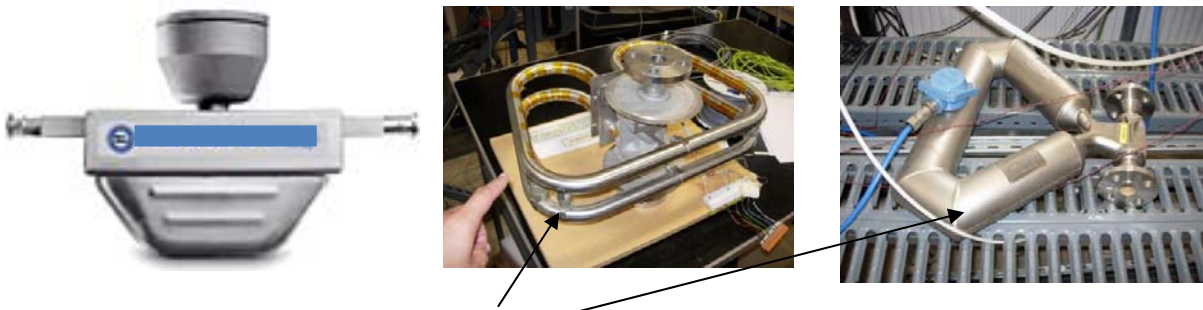


Figure 12. Examples of stainless steel tube Coriolis mass flow / density meters (23-25).

preventing these devices from wider use. These large industrial sensors sell for \$3,500 to more than \$20,000 (23-25). A MEMS chip-based sensor has a significant cost and size advantage over the larger, hand assembled steel tube flow and density sensors.

Since all Coriolis mass flow and density meters are vibratory devices, vibration sensitivity has been underlying problem with this technology. This is a critical problem for industrial, automotive and aerospace applications where shock and vibration are common place. Conventional metal tube Coriolis mass flow meters resonate at 100 to 1500 Hz (24,25), leaving them susceptible to the spectrum of common external mechanical vibration and shock frequencies which are under 2000Hz. To

examine the difference between the MEMS sensor in this study and a conventional steel tube and MEMS-based Coriolis mass flow sensor both were placed on a vibratory test stand and cycled from 10 Hz to 1000Hz starting at 0.5g and going to 2g acceleration while monitoring the zero flow rate output of a water filled tube. Figure 13 shows that the

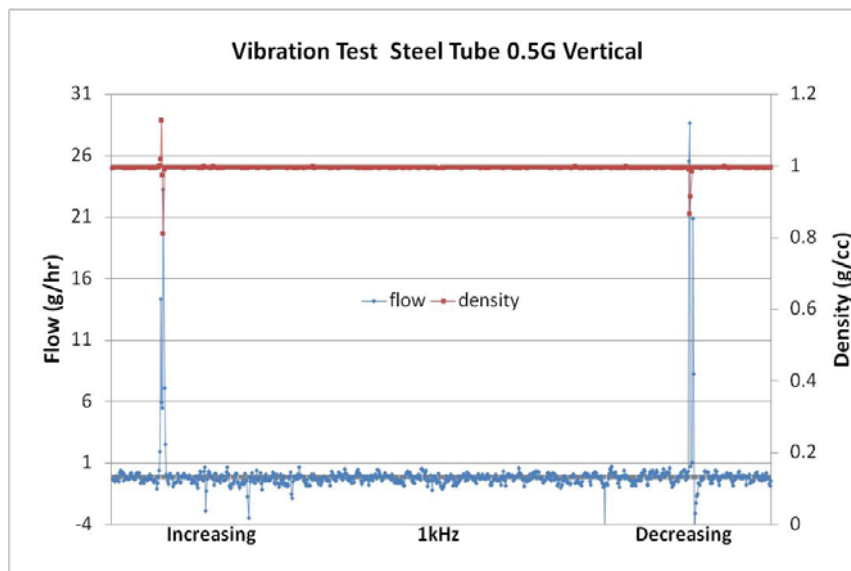


Figure 13. Flow and density errors in stainless steel tube Coriolis meters under vibration.

conventional steel Coriolis

meter had both large flow and density output spikes at its resonance frequency at very low accelerations, 0.5g. The silicon tube used in the MEMS sensor in this study has resonant frequencies ranging from 20KHz to 30KHz, well above what is typically experienced in an industrial, automotive or aerospace applications. The zero flow rate output of the MEMS tube was within a +/- 1 g/hr band at all external vibrational frequencies at 2 g. The density output of the MEMS sensor was not affected by vibration. This is an advantage for the MEMS-based Coriolis mass flow and density meters over conventional steel tube technology and can broaden the field of use to include applications with significant vibration and shock like the trucking and aerospace markets.

5. Conclusions

ISSYS is marketing new density and chemical concentration measurement technology that opens up capabilities for the fuel quality, custody transfer and blending markets. Petrochemicals, fuels, biofuels can be monitored for concentration, purity, water content and grade using density. Operating on the same principle as conventional steel Coriolis meters, the ISSYS sensing element is small enough to fit on your finger tip. This size advantage and its associated cost savings enables this sensing capability to be distributed across new areas in fuel and chemical management.

6. References Cited

1. W.Harrison, The role of Fischer Tropsch fuels for the US military, AFRL-06-0078, 2006
2. E.Frame et al., "Alternative fuels:Assessment of fisher-tropsch fuel for military use in 6.5L diesel engine," SAE Transaction, vol. 113, no. 2217, pp.1826-1842, 2004.
3. N.Clark et al., On-road use of Fischer-Tropsch diesel blends, SAE, paper no. 1999-01-2251, 1999.
4. K.Varde & C.Clarke, "A Comparison of Burn Characteristics and Exhaust Emissions From Off- Highway Engines Fueled By E0 and E85," SAE 2004-28-0045, (2004).
5. D.Nelson, S.Boyd, P.Hiester & S.Lawson, "Design and Development Process for the Equinox REV LSE E85 Hybrid Electric Vehicle," SAE 2006-01-0514, (2006).
6. K.Lundergaard, "Ford, GM Make Big Push to Promote Flex-Fuel Vehicles," WSJ, p.B1, Jan. 10, (2006).
7. L.Rother, "With Big Boost from Sugar Cane, Brazil is Satisfying Its Fuel Needs," NYT, p.A1, April 10, (2006).
8. "Ethanol Plants," <http://www.card.iastate.edu/research/bio/tools/ethanol.aspx>, May 2008.
- 9.L.Horkey, "Higher Blends," Ethanol Today, p.12-14, July 2007.
10. "Biofuels in the US Transportation Sector," Energy Information Administration, October 2007.
11. F. Alasfour, Butanol-a single cylinder engine study: engine performance, Intl. Jor. Energy Research, 21 (1997), pp.21-30.
12. "Biodiesel 2020: A global market survey," 2nd Ed. Emerging Markets Online, 2008.
13. M.Tat and J.Gerpen, Physical properties and composition detection of biodiesel fuel blends, Proc. 2002 ASAE intl. Mtg., Paper# 026084, July 2002.
14. J.Duban and R.Turner, On farm methods of biodiesel blend detection, 2006 ASABE Annual Intl. Meeting, Paper No. 0066239, Portland, OR, July, 2006.
15. D. Sparks, R. Smith, R. Schneider, J. Cripe, S. Massoud-Ansari, A. Chimbayo, N. Najafi, "A variable temperature, resonant density sensor made using an improved chip-level vacuum package," Sensors and Actuators A, vol. 107, pp.119-124, (2003)
16. D.Sparks, K.Kawaguchi, M.Yasuda, D.Riley, V.Cruz, N.Tran, A.Chimbayo, N.Najafi, "Embedded MEMS-based concentration sensor for fuel cell and biofuel applications," Sensors and Actuators A, vol. 145-146, pp.9-13, (2008).
17. D.Sparks, D.Goetzinger, D.Riley, N.Najafi, A by-pass sensor package design enabling the use of microfluidics in high flow rate applications, Proceedings of the 2006 ASME MEMS/NEMS Packaging Symposium, Chicago, IL, Nov. 2006.
18. D.Sparks, D.Riley, V.Cruz, N.Tran, A.Chimbayo, N.Najafi, K.Kawaguchi, M.Yasuda, "Embedded MEMS-based concentration sensor for improved active fuel cell performance, Transducers & Eurosensors'07, pp. 1911-1914, Lyon, France, June (2007).
19. D.Eddy and D.Sparks "Application of MEMS technology in automotive sensors and actuators," Proceedings IEEE, vol.86, no.8, pp.1747-1753, Aug. (1998).
20. J.Bacha et al., Diesel fuel refining and chemistry, Diesel Fuels Tech. Rev., FTR-2, 1998.
21. World Micro Fuel Cell Markets for Portable Devices, #A659-27, Frost & Sullivan Sept. (2004).
22. G.Jung, A.Su, C.Tu, F.Weng, "Effect of operating parameters on the DMFC performance," J.Fuel Cell Sci & Tech., vol. 2, pp.81-85, (2005).
23. Piechota, "The continuing Coriolis evolution," Flow Control, vol. 8, p.8,2002
24. N.Keita, "Behavior of straight pipe Coriolis mass flowmeters in the metering of gas:theoretical predictions with experimental verification," Flow Meas. Instrum. vol. 5, pp. 289-294, 1994.
25. A.Skea and A.Hall, "Effects of gas leaks in oil flow on single-phase flowmeters," Flow Meas. Instrum. vol. 10, pp.146-150, 1999.

For more information contact:

Integrated Sensing Systems (ISSYS)
391 Airport Industrial Dr., Ypsilanti, MI 48198
www.issys-mems.com
Tel: (734) 547-9896 Ext. 127
Fax: (734) 547-9964
Email: density@mems-issys.com



October 28, 2008